

По вопросам продаж и поддержки обращайтесь:

Архангельск (8182)63-90-72
Астана (7172)727-132
Астрахань (8512)99-46-04
Барнаул (3852)73-04-60
Белгород (4722)40-23-64
Брянск (4832)59-03-52
Владивосток (423)249-28-31
Волгоград (844)278-03-48
Вологда (8172)26-41-59
Воронеж (473)204-51-73
Екатеринбург (343)384-55-89

Иваново (4932)77-34-06
Ижевск (3412)26-03-58
Казань (843)206-01-48
Калининград (4012)72-03-81
Калуга (4842)92-23-67
Кемерово (3842)65-04-62
Киров (8332)68-02-04
Краснодар (861)203-40-90
Красноярск (391)204-63-61
Курск (4712)77-13-04
Липецк (4742)52-20-81

Магнитогорск (3519)55-03-13
Москва (495)268-04-70
Мурманск (8152)59-64-93
Набережные Челны (8552)20-53-41
Нижний Новгород (831)429-08-12
Новокузнецк (3843)20-46-81
Новосибирск (383)227-86-73
Омск (3812)21-46-40
Орел (4862)44-53-42
Оренбург (3532)37-68-04
Пенза (8412)22-31-16

Пермь (342)205-81-47
Ростов-на-Дону (863)308-18-15
Рязань (4912)46-61-64
Самара (846)206-03-16
Санкт-Петербург (812)309-46-40
Саратов (845)249-38-78
Севастополь (8692)22-31-93
Симферополь (3652)67-13-56
Смоленск (4812)29-41-54
Сочи (862)225-72-31
Ставрополь (8652)20-65-13

Сургут (3462)77-98-35
Тверь (4822)63-31-35
Томск (3822)98-41-53
Тула (4872)74-02-29
Тюмень (3452)66-21-18
Ульяновск (8422)24-23-59
Уфа (347)229-48-12
Хабаровск (4212)92-98-04
Челябинск (351)202-03-61
Череповец (8202)49-02-64
Ярославль (4852)69-52-93

Единый адрес: esu@nt-rt.ru | <http://epluse.nt-rt.ru>

HUMOR 20


High-precision Humidity Calibrator

The role of humidity calibrations that are accurate, reproducible, and documentable is becoming more and more important. ISO quality guidelines and regulations according to FDA guidelines in the pharmaceutical industry, etc., require that humidity instruments have a traceable, accurate calibration. The humidity calibrator HUMOR 20 developed by E+E is the ideal reference instrument for these requirements.

The HUMOR 20 can be used in the humidity range of 10-95% RH both for monitoring cylindrical sensors (transmitters, hand-held instruments,...) and also for monitoring instruments with cubic dimensions (data loggers, wall instruments,...). A temperature sensor integrated in the measurement chamber also permits the monitoring of an optional temperature output.

The HUMOR 20 is traceable to international standards and can be delivered with an official, internationally recognised OEKD calibration certificate. Due to its high accuracy, the HUMOR 20 is the basis for accredited calibration laboratories for relative humidity.

Based on its operating principle, the HUMOR 20 can be used under typical conditions in a laboratory climate. This means that expensive, fully air-conditioned rooms are not necessary. For operation HUMOR 20 requires only distilled water, filtered oil-free air with a pressure of 10 bar and a power supply between 90-230V AC. The specimen can be powered by 24V DC that is

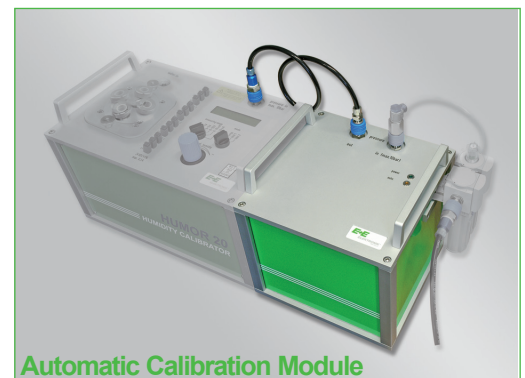


Open

The operation of the HUMOR 20 is based on a fundamental two-pressure process and thus is similar to instruments used in national bureaus for standards. Air or nitrogen at a pressure p_1 is led through a water-filled saturation chamber and saturated to 100% RH at p_1 . By means of a reduction valve, the saturated air is reduced to the ambient pressure p and fed into the measurement chamber. Due to the construction, the saturation chamber and the measurement chamber are at the same temperature. Under these conditions, the water-vapour partial pressure e_{ws} is reduced at the same ratio as the total pressure. Essentially, the following applies:

$$e = e_{ws} \cdot p / p_1$$

From this it follows that: $RH = e / e_{ws} = p / p_1$

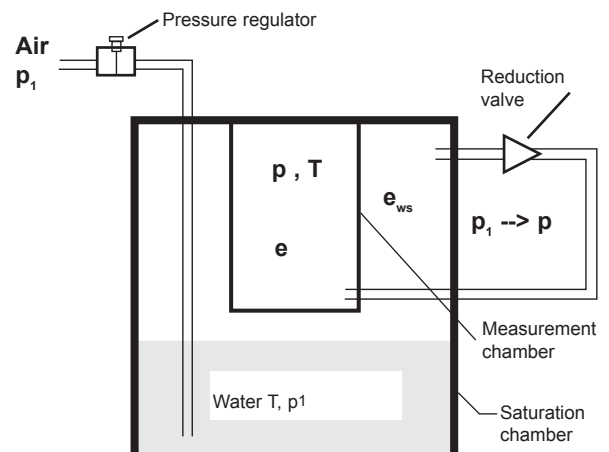

Schematic Illustration of a Two-pressure Reactor

Typical Applications

calibration laboratories
reference device
bureau of standards
manufacturers of measurement instruments

Features

highest accuracy
traceable calibration
independent of ambient temperature
easy handling
traceable to international standards
OEKD certificatable

Automatic Calibration Module

The optional available Automatic Calibration Module enables an automatic set point adjustment of the desired reference humidity. With the software, included in the scope of supply, checkpoints, stabilisation times, etc. can be set. Furthermore the instrument allows for an automatic print out of a calibration protocol for a transmitter with analogue standard interface.

Calibration and Adjustment using HUMOR 20

24V DC electrical supply for the test sample are provided directly at HUMOR 20.

Furthermore, four inputs for the voltage or current outputs of transmitters are available when using the Automatic Calibration Module for generating calibration protocols.

The software which is included in the scope of supply allows the user to record measurement values in a log file, to print out calibration protocols and to configure or to readjust the HUMOR 20.

Software - Features:

- Freely selectable numbers of measuring points and stabilisation times when using the Automatic Calibration Module
- Creation and print out of professional calibration protocols with:
 - Specimen number
 - Calibration date
 - Reference and actual values
- Temperature display can be switched between °C and °F
- 1-point customer humidity calibration of the HUMOR 20
- 6-point customer humidity calibration of the HUMOR 20
- 1-point customer temperature calibration
- Reset of HUMOR 20 to factory calibration



Technical Data


General

Function principle two-pressure-reactor

Working range 10...95% RH

Accuracy of measurement^{1) 2)}

(Traceable to international standards, administrated by NIST, PTB, BEV...)

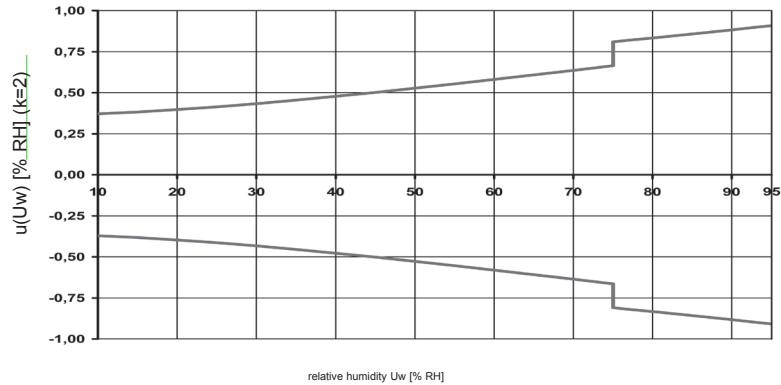

Accuracy temperature measurement in measuring chamber²⁾

typ. $\pm 0.3^{\circ}\text{C}$ ($\pm 0.54^{\circ}\text{F}$)

Power supply

90...230V AC

Work equipment

- compressed air, filtered and free of oil or nitrogen N_2 with max. 10bar (145psi)
- distilled water

Stabilisation time HUMOR 20

< 3 min/measuring point

Stabilisation time specimen

typ. 20 min/measuring point

Integrated power supply

24V DC, max. 200mA

Number of measuring inputs

4 (switchable between 4...20mA / 0...20mA / 0...1V / 0...5V / 0...10V)

Typ. error for display inputs

Voltage measuring: < 5mV

Current measuring: < 30 μA

Display

Dot-matrix display with backlight

Gas flow

3 l/min

for RH > 85% the gas flow is reduced to 1.5 l/min at 95% RH

Recommended interval for recalibration

1 year

Interface for PC connection

RS232 (COM port)

System requirements for software tools

MS Windows 2000 with SP 2 / Windows XP / Windows Vista / Windows 7

Environmental conditions

temperature: 10...40 $^{\circ}\text{C}$ (50...104 $^{\circ}\text{F}$)

humidity: 10...80% RH

Applied harmonised standards

EN 61000-6-3

EN 60068-2-6

EN 61000-6-2

EN 61010-1

EN 61326-1

EN 60068-2-29



Dimensions

400 x 260 x 240 mm (15.7 x 10.2 x 9.4")

Weight

HUMOR 20: about 23kg (51 lbs)

HUMOR 20 incl. aluminium transport case: about 36.5kg (80.5 lbs)

Measuring Chamber

The construction of the measuring chamber allows the calibration and adjustment of cylindrical sensor probes with a diameter of 8-25.5mm (0.3-1") (hand-held instruments, duct-mounted versions, ...) as well as of cubic measuring units (room transmitters, data loggers, ...) with maximum dimensions of 100x85x40mm (3.9x3.3x1.6") or 95x95x40mm (3.9x3.9x1.6").

By using the Plexiglas cover (standard supply), it is possible to calibrate and adjust compact room devices (e.g., the EE10) with the HUMOR 20.

The overall accuracy of the calibration is influenced by the absence of the metal cover. The additional error depends on the position of the specimen in the chamber as well as on the relative humidity.

1) The extended inaccuracy of measurement results from the standard inaccuracy increased by a multiplying factor of K=2.

2) Valid for metal covers for the measuring chambers

Accessories

Compressor with oil separator

Technical Data:

Max. operation pressure	12bar (174psi)
Supply voltage	100, 120, 200 or 230V AC // 50 or 60Hz
Noise level	45dB(A)/1m
Dimensions (l x w x h)	400 x 400 x 570 mm (15,74 x 15,74 x 22,44")
Weight	29kg (64lbs)



Optional covers for the measuring chambers

Various covers for the measuring chamber accommodate probes of all diameters available on the market.


With these covers up to four probes can be calibrated simultaneously.

SUITABLE FOR	NUMBER OF FEEDTHROUGHS	ORDER CODE
probe Ø 8 - 12mm (0.3 - 0.5")	3	HA020204
probe Ø 12 - 16mm (0.5 - 0.6")	2	HA020201
probe Ø 16 - 20.5mm (0.6 - 0.8")	1	HA020202
probe Ø 20.5 - 25.5mm (0.8 - 1")	1	HA020203
probe Ø 12mm (0.47 - 0.51")	4	HA020205
probe Ø 12 - 16mm (0.5 - 0.6")	4	HA020207
HUMLOG 10	-	HA020206
adapter for EE33-J ¹⁾	1	HA020401

1) only useable in combination with HA020204 or HA020201

Calibration certificate

To meet the requirements of Quality Management Systems such as ISO9001 regarding calibration and certification of measurement and test instrumentation, the HUMOR 20 is available with an official OEKD accredited calibration certificate.

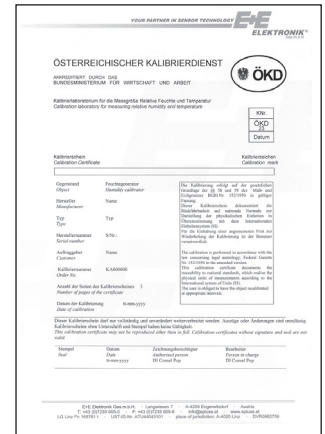


Automatic Calibration Module


For the fully automatic measurement of the characteristics of a transmitter.

Technical Data:

Weight	- weight of instrument: 9kg (20lbs) - instrument incl. aluminium transport case: 23kg (51lbs)
Dimensions	260x260x240mm (LxBxH); (10.2"x10.2"x9.4")
Supply	90...230V
Interface to PC	RS232 (COM Port)
Compressed air supply	min. 9.8bar (142psi); max. 12bar (174bar) oil-free filtered compressed air, max. size of particle: 5µm
Protection class	IP40
Scope of supply	- automatic calibration module - power supply cable IEC Europe (230V) - power supply cable IEC Northamerica (110V) - RS232 connection cable to Humor 20 - compressed air connection cable to Humor 20

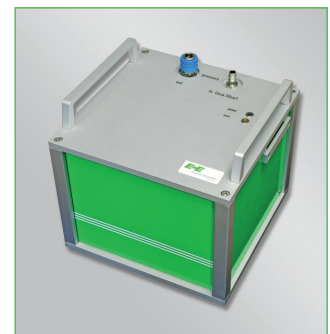

HUMOR 20 - Scope of Supply

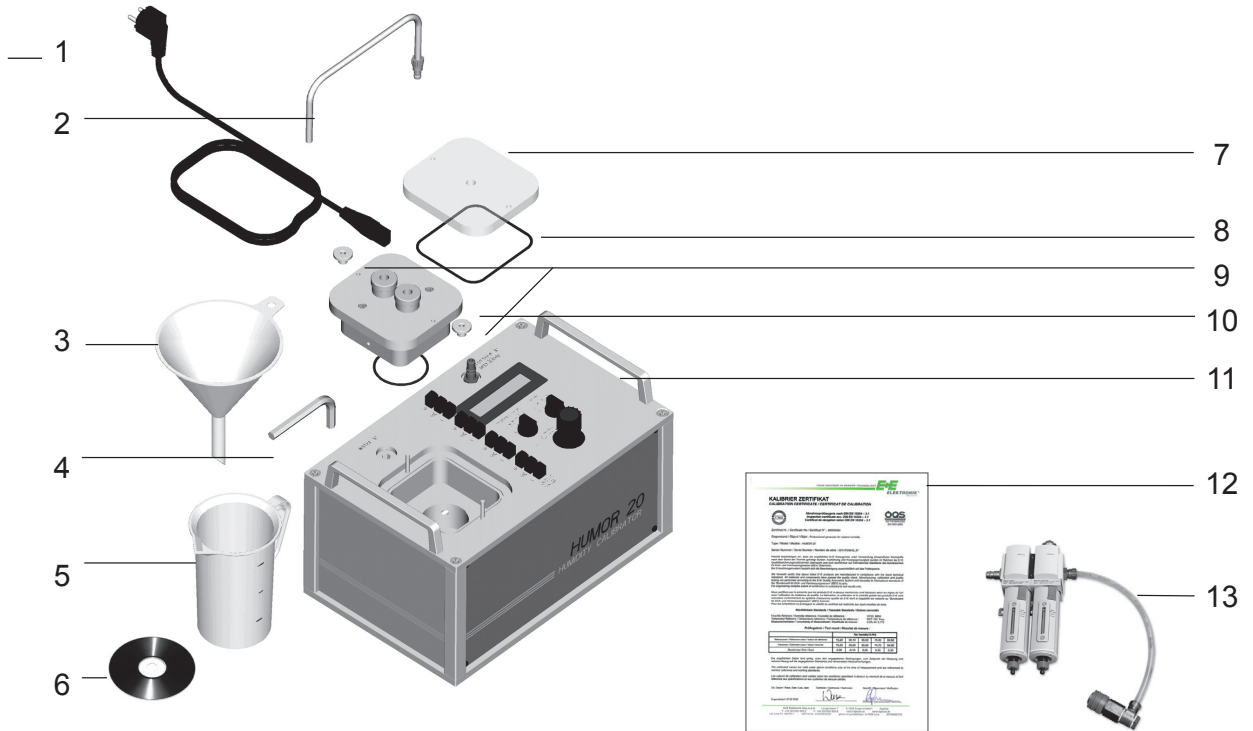

- 1 Power supply cable IEC Europe (230V) + power supply cable IEC Northamerica (110V)
- 2 Water drain pipe with connector
- 3 Funnel
- 4 Allen key (10mm / 0.4")
- 5 Measuring beaker
- 6 Measuring and calibration software
- 7 Plexiglas cover for room transmitter testing

- 8 O-ring for room transmitter
- 9 Knurled nut
- 10 Cover for measuring chamber (ordering code HA0202xx) (not included in the scope of supply HUMOR 20)
- 11 Fixing bracket for filter set (pre-mounted)
- 12 Works certificate acc. DIN EN 10204-3.1
- 13 Filter set with oil separator

Ordering Information

HUMIDITY CALIBRATOR

HUMOR 20	HUMOR20
Automatic Calibration Module	HA020301

COVER FOR MEASURING CHAMBER

Humor cover 12 - 16mm (0.5 - 0.6") plane	-	for 2 Probes	HA020201
Humor cover 16 - 20,5mm (0.6 - 0.8") plane	-	for 1 Probe	HA020202
Humor cover 20,5 - 25,5mm (0.8 - 1") plane	-	for 1 Probe	HA020203
Humor cover 8 - 12mm (0.3 - 0.5") plane	-	for 3 Probes	HA020204
Humor cover 12 - 13mm (0.5 - 0.52") conic	-	for 4 Probes	HA020205
Humor cover für HUMLOG 10	-	for 1 Probe	HA020206
Humor cover 12 - 16mm (0.5 - 0.6") bevelled	-	for 4 Probes	HA020207
Humor cover 16 - 20,5mm (0.6 - 0.8") bevelled	-	for 4 Probes	HA020208
Humor cover 30mm (1,2") plane	-	for 1 Probe	HA020209
Adapter for EE33 - modell J ¹⁾			HA020401

1) only useable in combination with HA020204 or HA020201

По вопросам продаж и поддержки обращайтесь:

Архангельск (8182)63-90-72
Астана (7172)727-132
Астрахань (8512)99-46-04
Барнаул (3852)73-04-60
Белгород (4722)40-23-64
Брянск (4832)59-03-52
Владивосток (423)249-28-31
Волгоград (844)278-03-48
Вологда (8172)26-41-59
Воронеж (473)204-51-73
Екатеринбург (343)384-55-89

Ижевск (4932)77-34-06
Ижевск (3412)26-03-58
Казань (843)206-01-48
Калининград (4012)72-03-81
Калуга (4842)92-23-67
Кемерово (3842)65-04-62
Киров (8332)68-02-04
Краснодар (861)203-40-90
Красноярск (391)204-63-61
Курск (4712)77-13-04
Липецк (4742)52-20-81

Магнитогорск (3519)55-03-13
Москва (495)268-04-70
Мурманск (8152)59-64-93
Набережные Челны (8552)20-53-41
Нижний Новгород (831)429-08-12
Новокузнецк (3843)20-46-81
Новосибирск (383)227-86-73
Омск (3812)21-46-40
Орел (4862)44-53-42
Оренбург (3532)37-68-04
Пенза (8412)22-31-16

Пермь (342)205-81-47
Ростов-на-Дону (863)308-18-15
Рязань (4912)46-61-64
Самара (846)206-03-16
Санкт-Петербург (812)309-46-40
Саратов (845)249-38-78
Севастополь (8692)22-31-93
Симферополь (3652)67-13-56
Смоленск (4812)29-41-54
Сочи (862)225-72-31
Ставрополь (8652)20-65-13

Сургут (3462)77-98-35
Тверь (4822)63-31-35
Томск (3822)98-41-53
Тула (4872)74-02-29
Тюмень (3452)66-21-18
Ульяновск (8422)24-23-59
Уфа (347)229-48-12
Хабаровск (4212)92-98-04
Челябинск (351)202-03-61
Череповец (8202)49-02-64
Ярославль (4852)69-52-93

Единый адрес: esu@nt-rt.ru | <http://epluse.nt-rt.ru>